




ENHANCING
your **OPTIONS**
FOR Restoring Flow

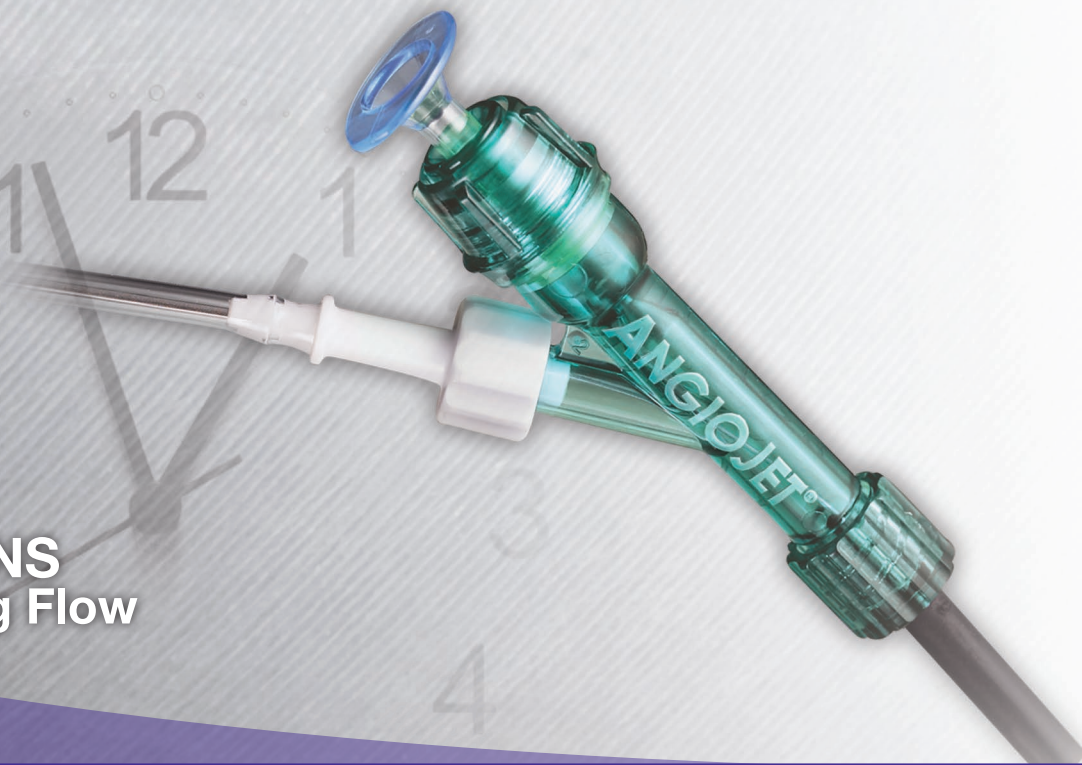

Rapid Thrombus Removal for Pulmonary Embolism


ANGIOJET®

PE
thrombectomy set

AngioJet® PE Thrombectomy Set

The *only* dedicated PE catheter for use with the AngioJet® System

Speed is important!


Life-threatening Pulmonary Embolism requires fast diagnosis and rapid haemodynamic stabilization.

European Society of Cardiology guidelines identify mechanical thrombectomy as “an alternative to thrombolysis when there are absolute contraindications, as an adjunctive therapy when thrombolysis has failed to improve haemodynamics or as an alternative to surgery if immediate access to cardiopulmonary bypass is unavailable...”¹

The AngioJet PE Thrombectomy Set is intended for use with the AngioJet System for removal of thrombus from main pulmonary and lobar arteries > 6mm.²

With over 600,000 catheters delivered worldwide, the AngioJet System offers rapid endovascular removal of thrombus.

AngioJet Thrombectomy has been proposed in several publications as a treatment option for patients with massive and submassive pulmonary embolism, with the potential of providing rapid and significant haemodynamic improvement with encouraging results at both early and long-term follow-up.^{3, 4, 5, 6}

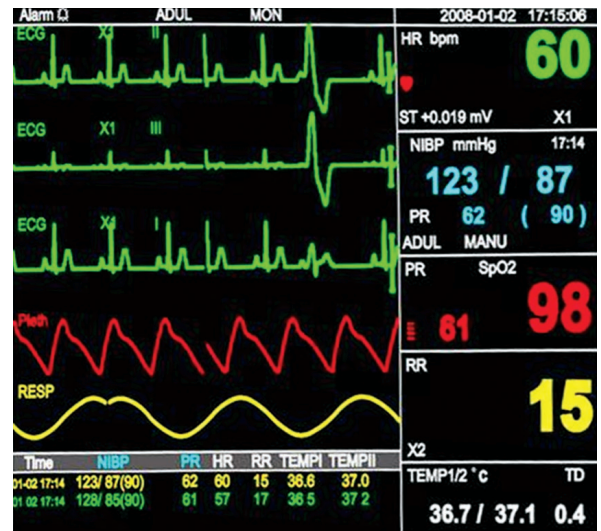

“Substantial improvement in pulmonary blood flow may result from what appears to be only modest angiographic change.” In fact, haemodynamic improvement may be a more indicative clinical parameter.⁷

Catheter Specifications

Min. Vessel Diameter	≥ 6mm
Low Profile Tip	2.0mm
Working Length	120cm
Max. Shaft Diameter	6F
Double Marker Band	15 mm
Guidewire Compatibility	OTW 0.035"
Guide Compatibility	8F > 0.086"
Sheath Compatibility	6F

Ordering Information

AngioJet PE Thrombectomy Set

Part number 107171-TAB

For use only with the AngioJet System

Bayer, the Bayer Cross, MEDRAD, AngioJet, Cross-Stream and Spiroflex are trademarks of the Bayer group of companies. Bayer © 2013
MEDRAD is part of Bayer HealthCare

Not approved in US. Indications, operating specifications and availability may vary by country. Check with local product representation and country-specific *Information for Use* for your country.

1. Torbicki A, Perrier A, Konstantinides S, Agnelli G, Galiè N, Pruszczyk P et al. Guidelines on the diagnosis and management of acute pulmonary embolism. The task force for the diagnosis and management of acute pulmonary embolism of the European Society of Cardiology (ESC). *European Heart Journal*, 2008;29:2276–2315.
2. AngioJet PE Thrombectomy Set Instructions for Use
3. Iskander A, Nayak A, Chauhan MS. Submassive pulmonary embolism and paradoxical embolic stroke treated with percutaneous rheolytic thrombectomy and closure of the patent foramen ovale. *Catheter Cardiovasc Interv* 2005;64(3):356–360.
4. Siablis D, Karnabatidis D, Katsanos K, Kagadis GC, Zabakis P, Hahalis G. AngioJet rheolytic thrombectomy versus local intrapulmonary thrombolysis in massive pulmonary embolism: A retrospective data analysis. *Journal of Endovascular Therapy* 2005;12(2):206–214.

5. Margheri M. Percutaneous rheolytic thrombectomy with AngioJet for pulmonary embolism: methods and results in the experience of a high-volume center. *Italian Journal of Cardiology* 2008;9(5):355–363

6. Arzamendi D, Bilodeau L, Ibrahim R, Noble S, Gallo R, Lavoie-L'Allier P et al. Role of rheolytic thrombectomy in massive pulmonary embolism with contraindication to systemic thrombolytic therapy. *EuroIntervention* 2009;5:716–721

7. Jaff M, McMurty S, Archer S, Cushman M, Goldenberg N, Goldhaber S et al. Management of massive and submassive pulmonary embolism, iliofemoral deep vein thrombosis, and chronic thromboembolic pulmonary hypertension. A scientific statement from the American Heart Association. *Circulation* 2011;123:1788–1830.



Bayer HealthCare

Manufacturer:

MEDRAD, INC.

One Medrad Drive
Indianola, PA 15051-0780 USA

Ph: +1 (412) 767-2400

Other: +1 (800) 633-7231

Fax: +1 (412) 767-4120

www.interventional.bayer.com

European Authorized Representative:

MEDRAD Europe B.V.

P.O. Box 205
6190 AE Beek

The Netherlands

Ph: +31 (0) 43-3585600



0086

4037-TAB 2/2013